

# NTP Synchronization SDS1004X-E

August 29, 2023


## Operating Tips - NTP Synchronization SDS1004X-E

The SDS1000X-E oscilloscope series supports date and time settings to allow data to be saved with the correct time of day. When it is necessary for multiple instruments to have the same date and time setting, it is convenient to synchronize the instruments to an NTP server. The SDS1xx4X-E series (4-channel) oscilloscopes allow synchronization to an NTP server using IP Address access.

The NTP feature was added in version 6.1.37R2 of the SDS1xx4X-E Firmware (4-Channel Models). Firmware update to latest version is recommended. The NTP function may also require an operating system update. Match version 6.1.37R10 with OS-V3. View all of the firmware and operating system updates here: <https://siglentna.com/service-and-support/firmware-software/digital-oscilloscopes/#sds1000x-e-series>

### Getting Connected

- Connect the SDS 1xx4X-E to the network and power it on.
- Press **Utility**. Then press the *Next Page* key to display Page 3 / 4
- Press *Date/Time* key for DATE/TIME menu.

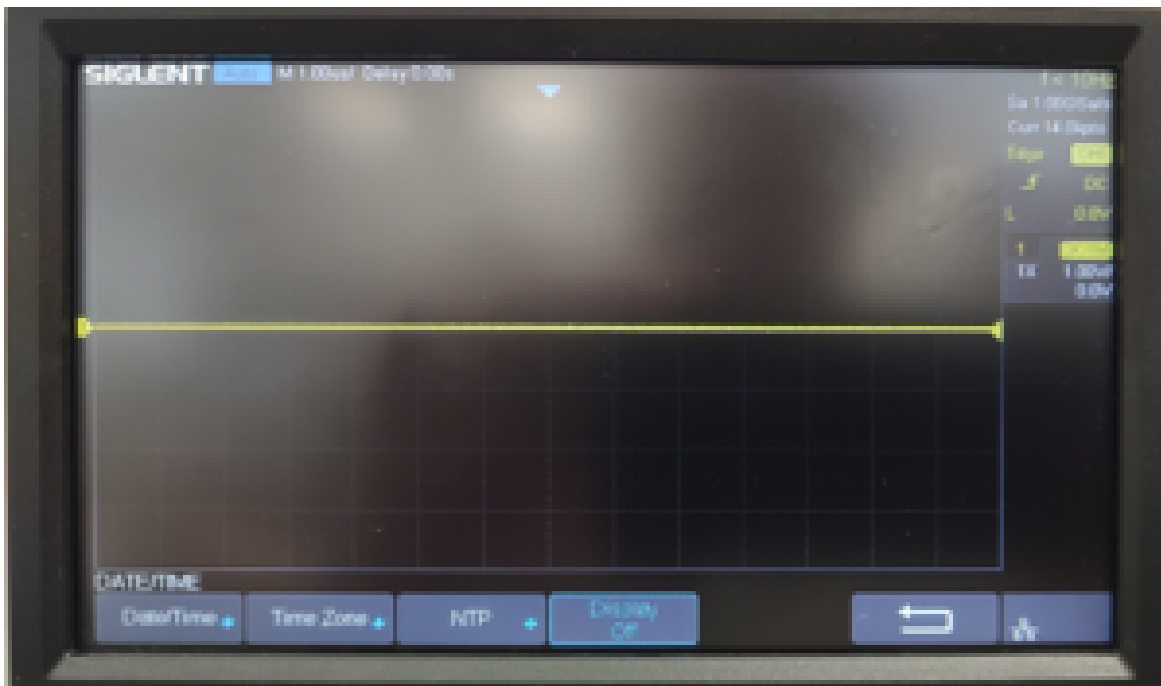


- Press *Display* key to change status from Off to On. This will show Date and Time in the upper-right corner of the screen. Before NTP is configured, date is default value and time is referenced to power on.




- Press *NTP* key to display the NTP menu and adjust the Server IP address. Rotate the **Adjust** knob to change value. Then press the **Adjust** knob to select the next part of the address.


The IP Address in this example is **132.163.97.1**

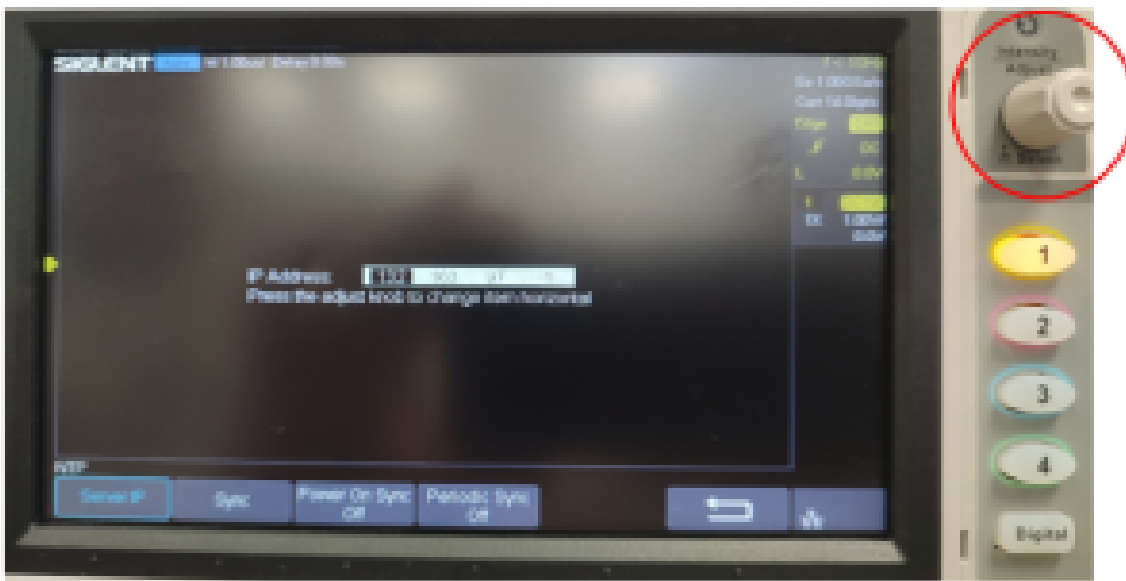


- After setting the IP Address, press *Sync*. The status message shown below appears at the bottom of the screen.




- Synchronization generally takes about 5 seconds. The status message below appears when synchronization is complete.



The Date/Time display is corrected after sync to NTP server.



- Multiple NTP servers are available in the United States. For a list of NIST NTP servers follow link: [NIST Internet Time Service](#). SDS1xx#4X-E Oscilloscopes are known to work with IP Address: **132.163.97.1**.
- Note that Date and Time settings are not maintained when the instrument is powered off, but synchronization to the NTP server can be set to happen automatically when the instrument is powered on:
  - From the Date/Time menu, press *NTP* key.
  - Press *Power On Sync* key to change status from Off to On. Now the instrument is set to synchronize to an NTP server following power-up.
  - (Optional) Press *Periodic Sync* key to change status from Off to On. This option invokes synchronization multiple times in one day. Synchronization can be set at intervals from 1 hour to 24 hours using the **Adjust knob**.
- To test, power cycle the instrument. The following message is displayed when this completes okay:





### **North American Headquarters**

SIGLENT Technologies America, Inc  
6557 Cochran Rd Solon, Ohio 44139  
Tel: 440-398-5800  
Toll Free: 877-515-5551  
Fax: 440-399-1211  
[info@siglent.com](mailto:info@siglent.com)  
[www.siglentamerica.com/](http://www.siglentamerica.com/)

### **European Sales Offices**

SIGLENT TECHNOLOGIES EUROPE GmbH  
Staetzlinger Str. 70  
86165 Augsburg, Germany  
Tel: +49(0)-821-666 0 111 0  
Fax: +49(0)-821-666 0 111 22  
[info-eu@siglent.com](mailto:info-eu@siglent.com)  
[www.siglenteu.com](http://www.siglenteu.com)

### **Asian Headquarters**

SIGLENT TECHNOLOGIES CO., LTD.  
Blog No.4 & No.5, Antongda Industrial Zone,  
3rd Liuxian Road, Bao'an District,  
Shenzhen, 518101, China.  
Tel: + 86 755 3661 5186  
Fax: + 86 755 3359 1582  
[sales@siglent.com](mailto:sales@siglent.com)  
[www.siglent.com/ens](http://www.siglent.com/ens)